

Al Takamul Company For Engineering Services

Quality Control – Iraq

Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

•Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: J	lune 3, 2024			Page 1 of 1
REQUEST NUMBER	:	By Mail	CUSTOMER DETAILS	
JOB NUMBER	:	QC/JN/24/00226	Name : Halliburton Worldwide IRAQ	(Sperry)
CERTIFICATE NUM	BER :	QC240603-12	Address : Western Burjesia, Oil Street, District Z	ubair-South Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description	: Dial Indic	ator Gauge				
Manufacturer	: Starrett					
Model	: 25-441					
Serial Number	: DIL-13					
SAP No	: 300098406	5				
Туре	: Analog					
Range	: 0	to		1 inch		2004 B 1004 B 100
Calibration Range	: 0	to		1 inch		
Readability	: 0.001"					
As Found	: In Toleran	ce				
Calibration Date	: June 3, 202	24				
Calibration Due	: 02 June 20)25				
Last Calibration	: June 5, 202	23				
ENVIRONMENTAL CON	DITIONS DU	JRING TEST	[
Ambient Temperature :	22.	$0 \pm 2^{\circ}C$	Humidity	:	$40.0~\pm 5~\%~RH$	

CALIBRATION METHOD

The above equipment has been calibrated in accordance with ASME B89.1.10M-2001

The reported uncertainty is the expanded uncertainty with k=2 according to the

ISO/IEC "Guide to the expansion of uncertainty in measurement" providing a level of confidence of approximately 95%.


REFERENCE EQUIPMENT USED :

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	DUE DATE
Gauge Block Set	87300	Mitutoyo / 99MAK004B2	November 15, 2023	November 14, 2024

CALIBRATION TEST RESULTS

Ref. Standard Values (A)	Measured Values on Unit Under Calibration (M)	Deviation (D=M-A)	Expanded Uncertainty (U)
inch	inch	inch	±inch
0.000	0.000	0.000	0.000
0.200	0.200	0.000	0.001
0.500	0.500	0.000	0.001
0.800	0.801	0.001	0.001
1.000	1.001	0.001	0.001

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

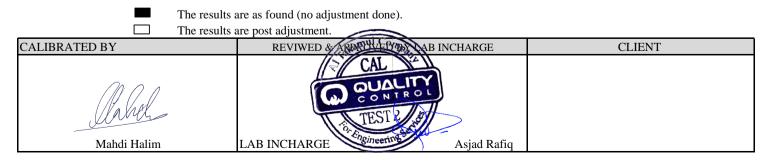

Corporate

artnei



150

9001



