

Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1


REQUEST NUMBER : By Contract JOB NUMBER : QC-CAL-25259 CERTIFICATE NUMBER : QC-CAL-25259-01	APPROVED BY LAB INCHARGE QC
--	------------------------------------

CUSTOMER DETAILS

Name : SLB Basra (Testing)
Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
Manufacturer : Badotherm
Model : NA
Serial Number : 24509-7
Type : Analog
Location : ESD-CD-847
Range : 0 to 400 bar
Calibrated Range : 0 to 400 bar
Resolution : 5 bar
Accuracy : 1.0
Tolerance : ± 1.0 % of Full Scale
As found : In Tolerance
Calibrated By : Hussein Alaa
Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C **Humidity** : 44.0 ± 5 % RH **Atm. Pressure** : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
bar	bar	bar	±
0	0	0	0.0
100	99.9	0.13	0.03
200	200.3	-0.30	-0.08
300	300.5	-0.54	-0.14
400	401.0	-1.00	-0.25

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.


Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

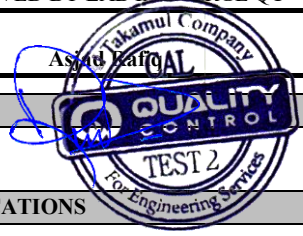REQUEST NUMBER : By Contract JOB NUMBER : QC-CAL-25259 CERTIFICATE NUMBER : QC-CAL-25259-02	APPROVED BY LAB INCHARGE QC 
--	--

CUSTOMER DETAILS

Name : SLB Basra (Testing)
Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
Manufacturer : Badotherm
Model : NA
Serial Number : 24509-8
Type : Analog
Location : ESD-CD-847
Range : 0 to 400 bar
Calibrated Range : 0 to 400 bar
Resolution : 5 bar
Accuracy : 1.0
Tolerance : ± 1.0 % of Full Scale
As found : In Tolerance
Calibrated By : Hussein Alaa
Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C **Humidity** : 44.0 ± 5 % RH **Atm. Pressure** : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
bar	bar	bar	±
0	0	0	0.0
100	99.7	0.27	0.07
200	199.8	0.20	0.05
300	300.3	-0.28	-0.07
400	400.5	-0.50	-0.13

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.

Certificate of Calibration


Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER	: By Contract	APPROVED BY LAB INCHARGE QC
JOB NUMBER	: QC-CAL-25259	
CERTIFICATE NUMBER	: QC-CAL-25259-03	



CUSTOMER DETAILS

Name : SLB Basra (Testing)
 Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
 Manufacturer : Gesa
 Model : NA
 Serial Number : CAL-SLB-03
 Type : Analog
 Location : ESD-CD-847
 Range : 0 to 150 psi
 Calibrated Range : 0 to 150 psi
 Resolution : 2 psi
 Accuracy : 1.6
 Tolerance : ± 1.6 % of Full Scale
 As found : In Tolerance
 Calibrated By : Hussein Alaa
 Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C Humidity : 44.0 ± 5 % RH Atm. Pressure : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
psi	psi	psi	±
0	0	0	0.0
40	40.3	-0.30	-0.20
80	80.2	-0.24	-0.16
120	120.4	-0.36	-0.24
160	160.4	-0.40	-0.27

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.


Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER : By Contract JOB NUMBER : QC-CAL-25259 CERTIFICATE NUMBER : QC-CAL-25259-04	APPROVED BY LAB INCHARGE QC 
--	--

CUSTOMER DETAILS

Name : SLB Basra (Testing)
Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
Manufacturer : SIMGA
Model : NA
Serial Number : CAL-SLB-01
Type : Analog
Location : ESD-CD-847
Range : 0 to 10 bar
Calibrated Range : 0 to 10 bar
Resolution : 0.5 bar
Accuracy : 1.0
Tolerance : ± 1.0 % of Full Scale
As found : In Tolerance
Calibrated By : Hussein Alaa
Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C **Humidity** : 44.0 ± 5 % RH **Atm. Pressure** : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
bar	bar	bar	±
0	0	0	0.0
2.5	2.50	0.00	-0.03
5.0	5.01	-0.01	-0.10
7.5	7.51	-0.01	-0.13
10.0	10.02	-0.02	-0.18

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.

Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com


Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER : By Contract JOB NUMBER : QC-CAL-25259 CERTIFICATE NUMBER : QC-CAL-25259-05	APPROVED BY LAB INCHARGE QC
--	------------------------------------

CUSTOMER DETAILS

Name : SLB Basra (Testing)
Address : North Rumaila Base south Iraq



EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
Manufacturer : SIMGA
Model : NA
Serial Number : CAL-SLB-02
Type : Analog
Location : ESD-CD-847
Range : 0 to 10 bar
Calibrated Range : 0 to 10 bar
Resolution : 0.5 bar
Accuracy : 1.0
Tolerance : ± 1.0 % of Full Scale
As found : In Tolerance
Calibrated By : Hussein Alaa
Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C **Humidity** : 44.0 ± 5 % RH **Atm. Pressure** : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
bar	bar	bar	±
0	0	0	0.0
2.5	2.49	0.01	0.10
5.0	5.00	0.00	0.05
7.5	7.51	-0.01	-0.08
10.0	10.02	-0.02	-0.15

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.



Certificate of Calibration


Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER	: By Contract	APPROVED BY LAB INCHARGE QC
JOB NUMBER	: QC-CAL-25259	
CERTIFICATE NUMBER	: QC-CAL-25259-06	



CUSTOMER DETAILS

Name : SLB Basra (Testing)
 Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
 Manufacturer : MC
 Model : NA
 Serial Number : CAL-SLB-04
 Type : Analog
 Location : ESD-CD-847
 Range : 0 to 1 MPa
 Calibrated Range : 0 to 1 MPa
 Resolution : 0.02 MPa
 Accuracy : ± 2.5 % of Full Scale
 Tolerance : ± 2.5 % of Full Scale
 As found : In Tolerance
 Calibrated By : Hussein Alaa
 Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C Humidity : 44.0 ± 5 % RH Atm. Pressure : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
MPa	MPa	MPa	±
0	0	0	0.0
0.25	0.251	-0.001	-0.10
0.50	0.502	-0.001	-0.15
0.75	0.752	-0.002	-0.22
1.00	1.002	-0.002	-0.20

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.


Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER : By Contract JOB NUMBER : QC-CAL-25259 CERTIFICATE NUMBER : QC-CAL-25259-07	APPROVED BY LAB INCHARGE QC 
--	--

CUSTOMER DETAILS

Name : SLB Basra (Testing)
Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : Pressure Gauge
Manufacturer : MC
Model : NA
Serial Number : CAL-SLB-05
Type : Analog
Location : ESD-CD-847
Range : 0 to 160 psi
Calibrated Range : 0 to 160 psi
Resolution : 5 psi
Accuracy : 2.5
Tolerance : ± 2.5 % of Full Scale
As found : In Tolerance
Calibrated By : Hussein Alaa
Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- 1 No adjustments were made prior to calibration.
- 2 Overload test was not performed.
- 3 No accessories were fitted.
- 4 Values were rounded in computation.

ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 2°C **Humidity** : 44.0 ± 5 % RH **Atm. Pressure** : 1011.0 ± 10 hPa

CALIBRATION METHOD

The above equipment has been calibrated in accordance with Calibration Procedure QC/CP/R/03 Rev. 01
 The above instrument has been calibrated in increasing and decreasing pressure mode using a Digital Pressure Calibrator as the reference standard having traceability to Internationally recognised standards.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	468802	AMETEK / XP2i	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Error Percentage
psi	psi	psi	±
0	0	0	0.0
40.0	40.11	-0.11	-0.07
80.0	80.17	-0.17	-0.11
120.0	120.26	-0.26	-0.16
160.0	160.35	-0.35	-0.22

Calibration results were found to conform as per specified accuracy requirements. Above Instrument has **PASSED** its Calibration.

- The results are as found (no adjustment done).
 The results are post adjustment.

Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER	: By Contract	APPROVED BY LAB INCHARGE QC
JOB NUMBER	: QC-CAL-25259	
CERTIFICATE NUMBER	: QC-CAL-25259-08	



CUSTOMER DETAILS

Name : **slb Basra (Testing)**
 Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : **Pressure Relief Valve**
 Manufacturer : NA
 Model : NA
 Serial Number : TC119401007
 Set/Pressure : 3100 psi
 Location : ESD-CD-847
 Tolerance : ±3 %
 Calibrated By : Hussein Alaa
 Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 1°C Humidity : 44.0 ± 5 % RH Atm. Pressure : 1011.0 ± 10 hPa

CALIBRATION METHOD

Standard Method API 527 was used to test the unit under test. Test pressure was applied on inlet of unit under test and test was repeated 3 times. Identical repetitions were carried out as recommended in used standard.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	1505119397	Sino Instruments / HS108	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Tolerance Limit
psi	psi	psi	± psi
3100	3112	-12	93.00

Results :

The above Value Indicates That the Instrument complies with the Specified Maximum Permissible error tolerance. At The Time of Calibration. and ready for use.

DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- The results relate to measurements taken at nominal value only.
- Adjustments were made prior to calibration.
- Accessories were fitted.

~ END OF DOCUMENT ~

Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER	: By Contract	APPROVED BY LAB INCHARGE QC
JOB NUMBER	: QC-CAL-25259	
CERTIFICATE NUMBER	: QC-CAL-25259-09	



CUSTOMER DETAILS

Name : **slb Basra (Testing)**
 Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : **Pressure Relief Valve**
 Manufacturer : NA
 Model : NA
 Serial Number : TC119401005
 Set/Pressure : 3100 psi
 Location : ESD-CD-847
 Tolerance : ±3 %
 Calibrated By : Hussein Alaa
 Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 1°C Humidity : 44.0 ± 5 % RH Atm. Pressure : 1011.0 ± 10 hPa

CALIBRATION METHOD

Standard Method API 527 was used to test the unit under test. Test pressure was applied on inlet of unit under test and test was repeated 3 times. Identical repetitions were carried out as recommended in used standard.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	1505119397	Sino Instruments / HS108	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Tolerance Limit
psi	psi	psi	± psi
3100	3108	-8	93.00

Results :

The above Value Indicates That the Instrument complies with the Specified Maximum Permissible error tolerance. At The Time of Calibration. and ready for use.

DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- The results relate to measurements taken at nominal value only.
- Adjustments were made prior to calibration.
- Accessories were fitted.

~ END OF DOCUMENT ~



Corporate Partner
Full Member

Address : North Rumaila, Al Takamul Yard
 Contact : +9647810009138

Certificate of Calibration

Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER	: By Contract	APPROVED BY LAB INCHARGE QC
JOB NUMBER	: QC-CAL-25259	
CERTIFICATE NUMBER	: QC-CAL-25259-10	



CUSTOMER DETAILS

Name : **slb Basra (Testing)**
Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : **Pressure Relief Valve**
Manufacturer : NA
Model : NA
Serial Number : 33675
Set/Pressure : 100 psi
Location : ESD-CD-847
Tolerance : ±2 %
Calibrated By : Hussein Alaa
Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 1°C Humidity : 44.0 ± 5 % RH Atm. Pressure : 1011.0 ± 10 hPa

CALIBRATION METHOD

Standard Method API 527 was used to test the unit under test. Test pressure was applied on inlet of unit under test and test was repeated 3 times. Identical repetitions were carried out as recommended in used standard.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	1505119397	Sino Instruments / HS108	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Tolerance Limit
psi	psi	psi	± psi
100	101.2	-1.2	2.00

Results :

The above Value Indicates That the Instrument complies with the Specified Maximum Permissible error tolerance.
At The Time of Calibration. and ready for use.

DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- The results relate to measurements taken at nominal value only.
- Adjustments were made prior to calibration.
- Accessories were fitted.

~ END OF DOCUMENT ~

Certificate of Calibration


Al Takamul Yard, North Rumailah South Iraq

• Phone : +964 7810009138 • www.qualitycontrol-iraq.com • E-mail: op@qualitycontrol-iraq.com

Date of Issue: July 12, 2025

Page 1 of 1

REQUEST NUMBER	: By Contract	APPROVED BY LAB IN CHARGE QC
JOB NUMBER	: QC-CAL-25259	
CERTIFICATE NUMBER	: QC-CAL-25259-11	



CUSTOMER DETAILS

Name : **slb Basra (Testing)**
 Address : North Rumaila Base south Iraq

EQUIPMENT IDENTIFICATION AND SPECIFICATIONS

Description : **Pressure Relief Valve**
 Manufacturer : NA
 Model : NA
 Serial Number : 34223
 Set/Pressure : 100 psi
 Location : ESD-CD-847
 Tolerance : ±2 %
 Calibrated By : Hussein Alaa
 Calibration Date : July 12, 2025
Calibration Due : July 11, 2026



ENVIRONMENTAL CONDITIONS DURING TEST

Ambient Temperature : 25.0 ± 1°C Humidity : 44.0 ± 5 % RH Atm. Pressure : 1011.0 ± 10 hPa

CALIBRATION METHOD

Standard Method API 527 was used to test the unit under test. Test pressure was applied on inlet of unit under test and test was repeated 3 times. Identical repetitions were carried out as recommended in used standard.

REFERENCE EQUIPMENT USED

DESCRIPTION	SERIAL NO.	MAKE / MODEL	CALIBRATION DATE	CALIBRATION DUE DATE
Digital Pressure Gauge	1505119397	Sino Instruments / HS108	5 Nov, 2024	4 Nov, 2025

CALIBRATION TEST RESULTS

Measured Values on Unit Under Calibration (M)	Ref. Standard Values (A)	Deviation (D=M-A)	Tolerance Limit
psi	psi	psi	± psi
100	99.2	0.8	2.00

Results :

The above Value Indicates That the Instrument complies with the Specified Maximum Permissible error tolerance. At The Time of Calibration. and ready for use.

DEVIATION FROM STANDARD METHOD : None

REMARK (S) :

- The results relate to measurements taken at nominal value only.
- Adjustments were made prior to calibration.
- Accessories were fitted.

~ END OF DOCUMENT ~



Corporate Partner
Full Member

Address : North Rumaila, Al Takamul Yard
 Contact : +9647810009138